Fast and stable | Efficient and uniform | The instrument is easy to operate

360 cryolipolysis

Operation instruction



Catalog

Product Introduction

Working Principle 01

Product Parameter 01

Product Structure Introduction 02

Instruction for use

Interface Introduction 04

Parameters Setting 08

Intended Users 09

Contraindications 09

Precautions 10

Accossories List 10

Product introductio

360 cryolipolysis

1. The negative pressure suction provides 360-degree comprehensive cooling and heating, allowing the freezing energy to reach as low as -10℃ and the heating energy up to 45℃. The system includes four operational cycling modes, enabling the adjustment of energy levels based on the treatment situation.

2. Eight different specifications of cryotherapy head templates are available for switching, including a mini version of the handpiece, suitable for treating individuals of different body types and various areas. This integrated device combines seven major technologies: cryotherapy, negative pressure, thermal energy, 40K, body RF, facial RF, and light sculpting. It adopts a non-invasive operating approach, making it a more intelligent and technologically advanced instrument.

Working principle

Utilizing precise and professional negative pressure technology, triglycerides undergo a phase transition from liquid to solid when fat cells in the targeted area are cooled to a specific temperature. Once crystallized, these fat cells progressively undergo apoptosis and are subsequently eliminated from the body through natural metabolism, effectively achieving weight loss objectives. The procedure is swift, and recovery is rapid, resulting in a well-proportioned and slender body shape for the individual seeking beauty enhancement.

Product specifications

Input Voltage	AC220V±10%、50HZ	Rated power	2000w
Vacuum	0-80Kpa	Handpiece Temperature	-10~45C
Lipo Laser Power	100mw/pcs	40K frequency	40KHz
RFfrequency	5MHz	Screen size	12.1
GW	70.65KG	Package	Wooden case

Product introductio

Product Structure Introduction

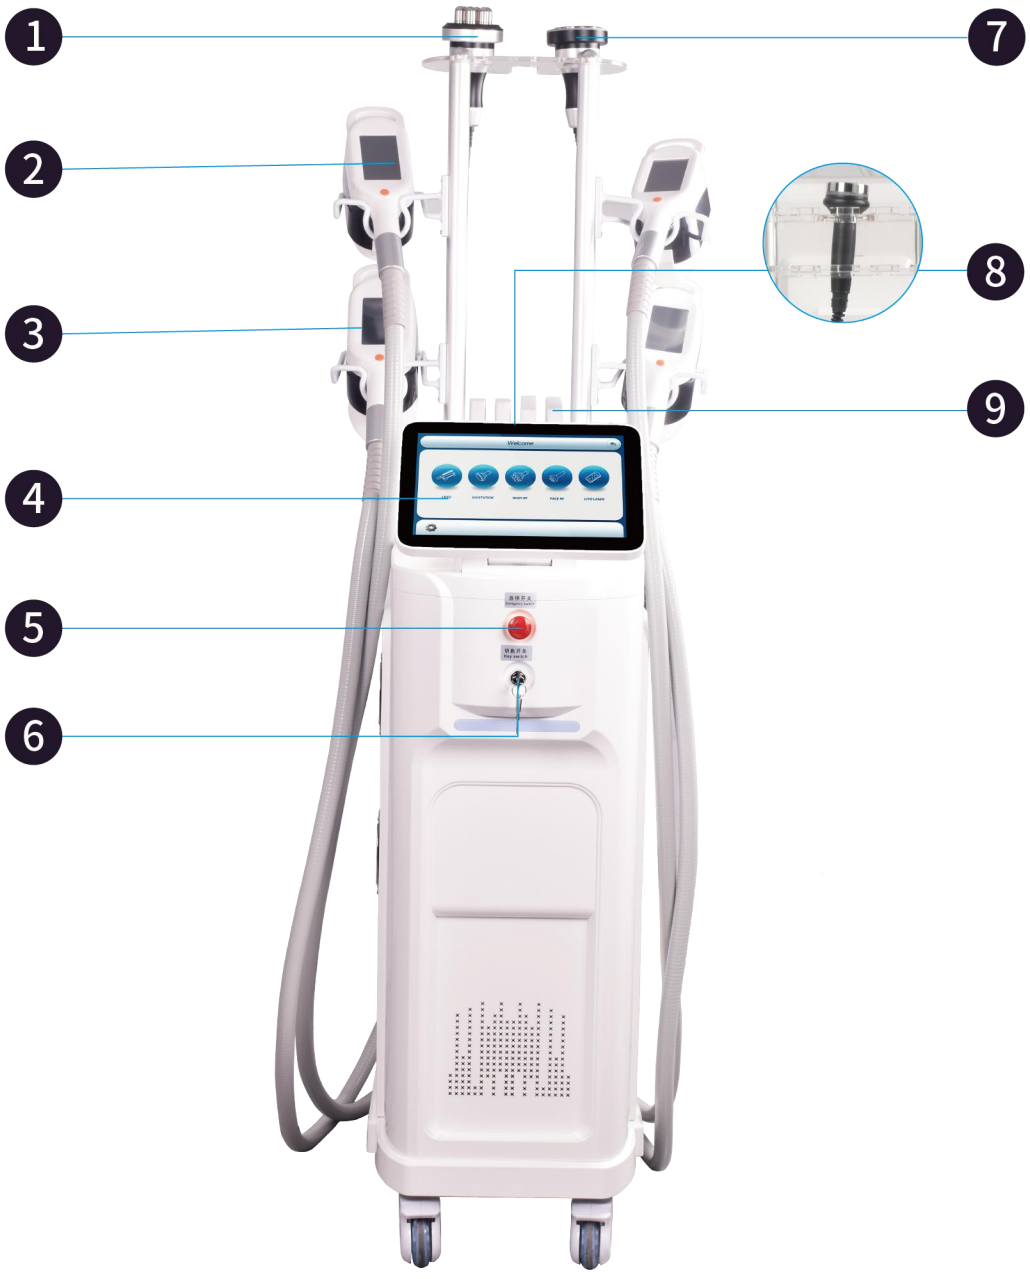

The front of machine
(Product in kind prevails)

1 RF Body Handle
2 Cryo Handle-M
3 Cryo Handle-L
4 HD screen
5 Emergency Button
6 key switch
7 40KHz Cavitation
8 Lipo L
9 Energy Tube

Product introductio

Structure introduction

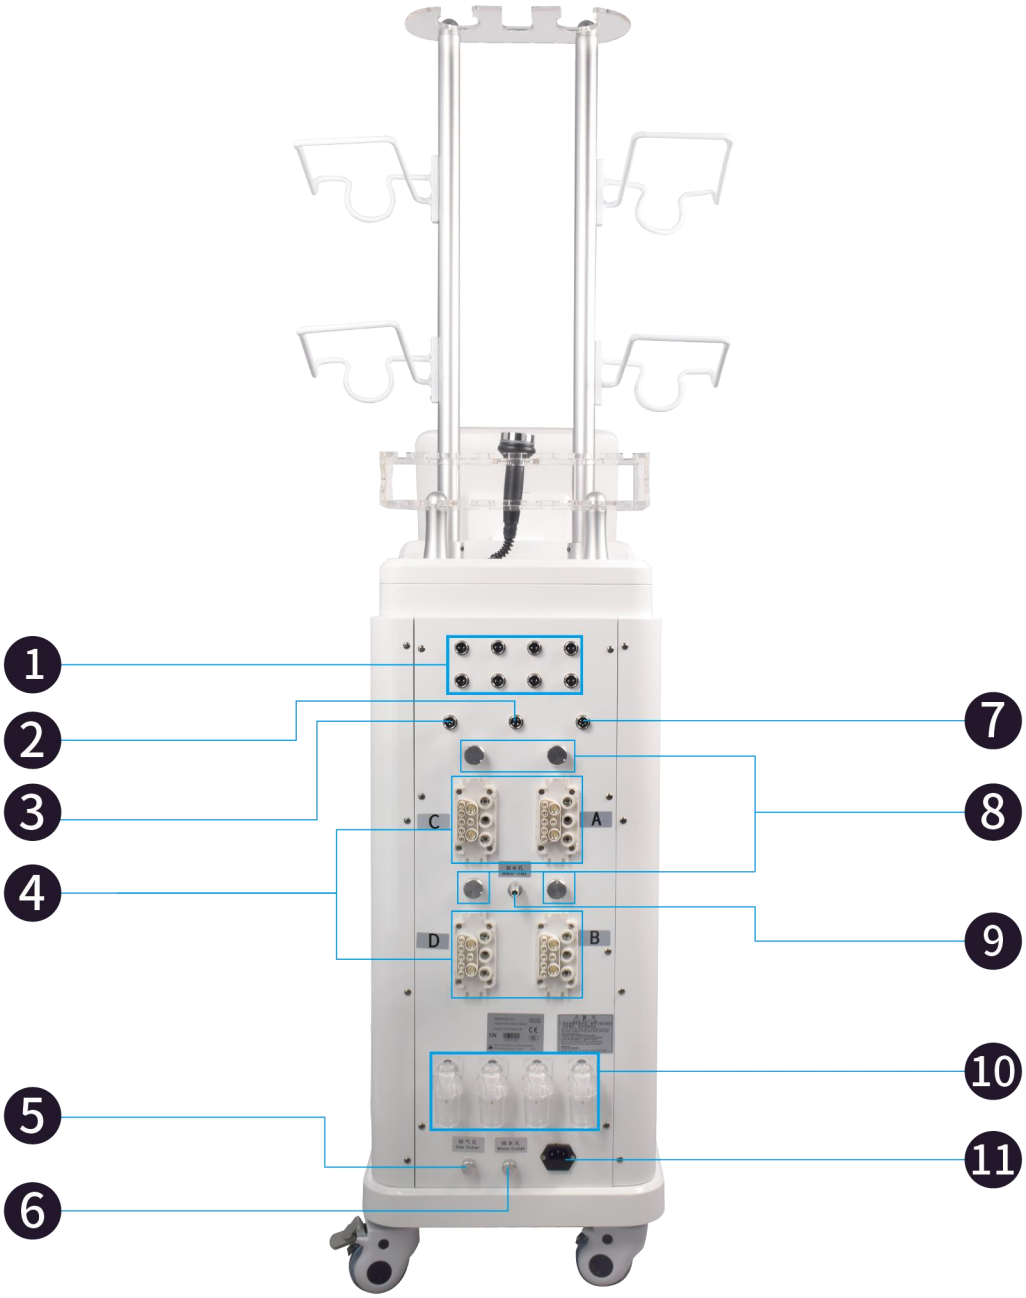

The back of machine
(Product in kind prevails)

1. Lipo Laser Socket
2. RF-face Socket
3. RF-body Socket
4. Cryo Socket
5. Vent
6. Water Outlet
7. 40K Socket
8. Pressure Regulator Valve
9. Water Inlet
10. Filter
11. Power Core Socket

Interface Introduction

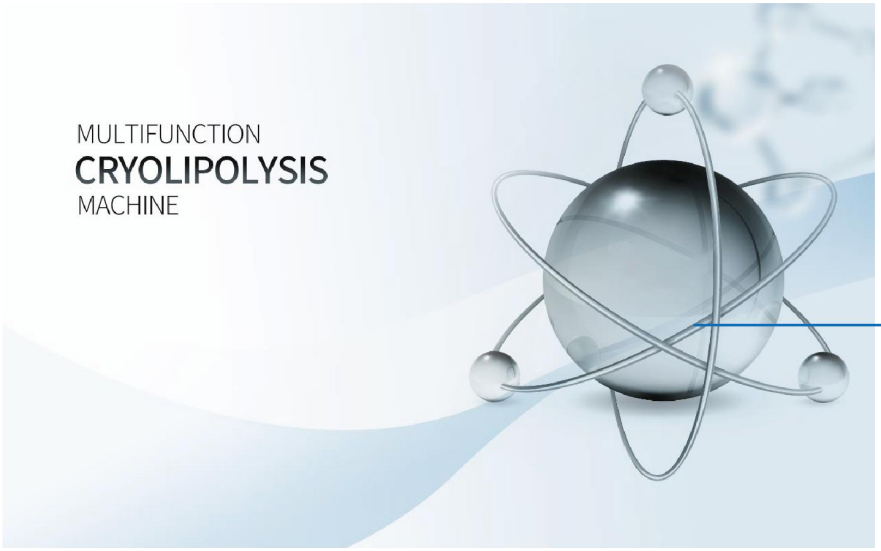

(1-1)

Boot Screen, click to enter



(1-2)

（1-2）Function Select Interface
The parameters for the cryo handle can be configured in the background by clicking on 'Setting' button and then entering the (1-3) interface. Once set, there is no need to configure the parameters separately during operation

Instruction for use

Interface introduction

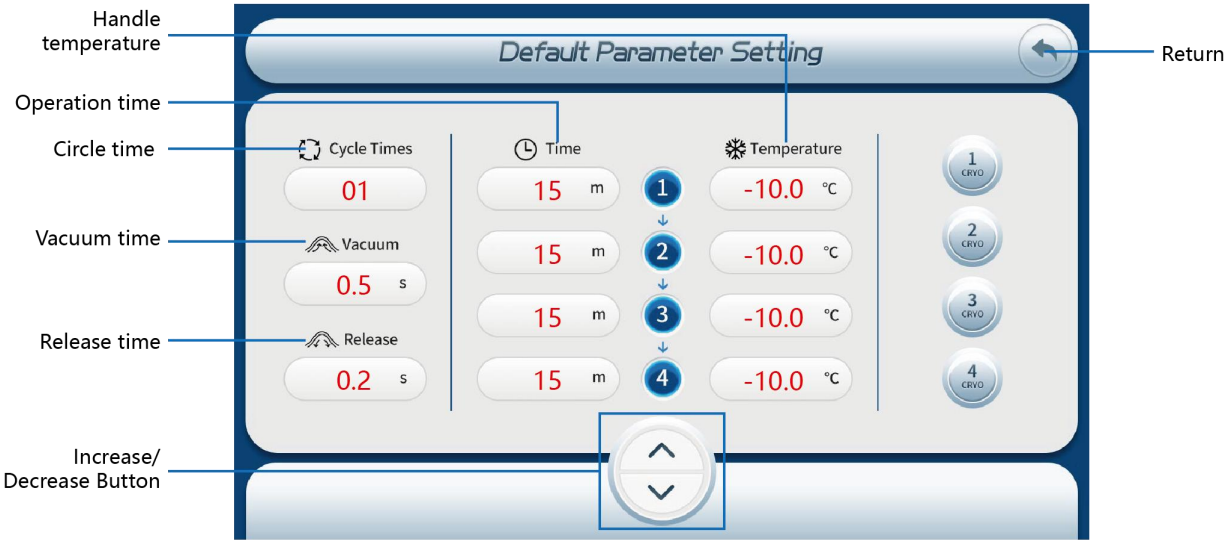

(2-1)

Page(2-) is the parameter setting interface for the cryotherapy mode. Set the parameters according to the above values, and these settings apply to each handle. Click 'Return' button to go back to the (2-2) interface

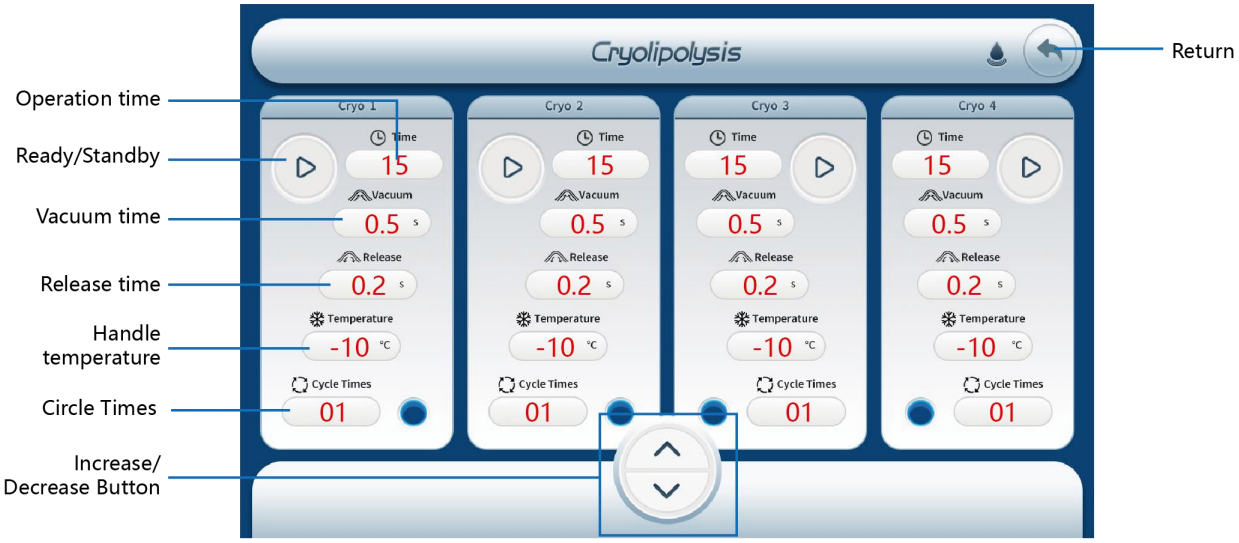

(2-2)

Click on the cryo handle button to enter (2-2). The displayed parameters on the interface reflect the values configured in the background. You can proceed with the operation directly by pressing the start button, or adjust them according to the customer's specific needs

Instruction for use

Interface introduction

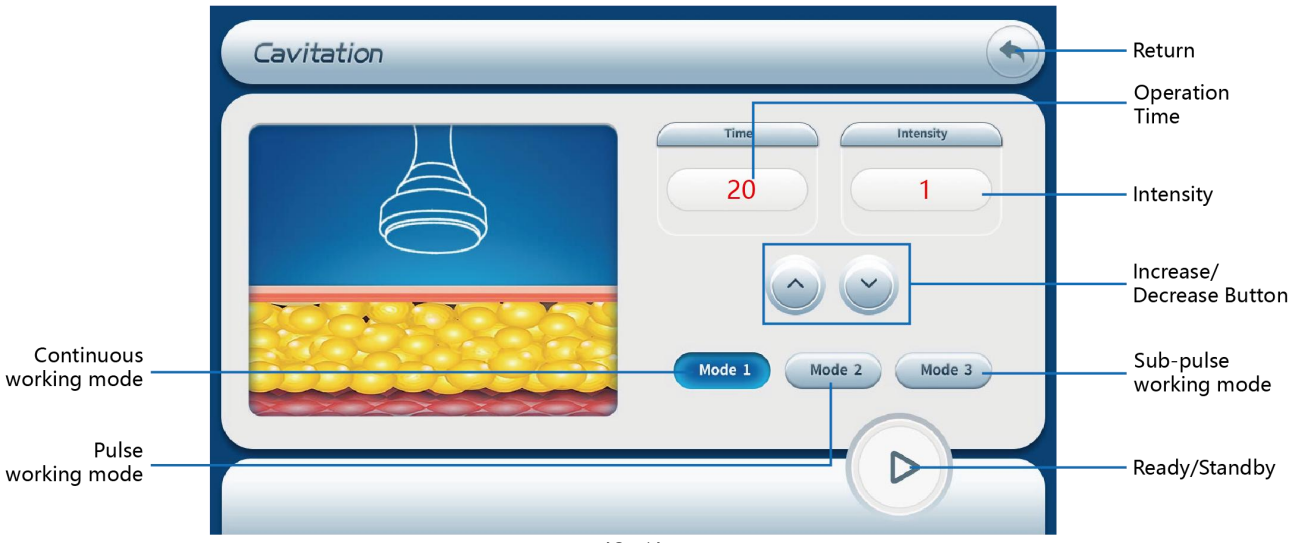

(3-1)

Click the 40K button on the (1-2) interface to enter the (3-1) interface. It is recommended to set the time between 20-30 minutes, starting the energy from level 1. Adjust the energy level based on the customer's comfort. Mode 1 is the default mode, and you can also choose different modes based on the actual situation. Click start to begin.

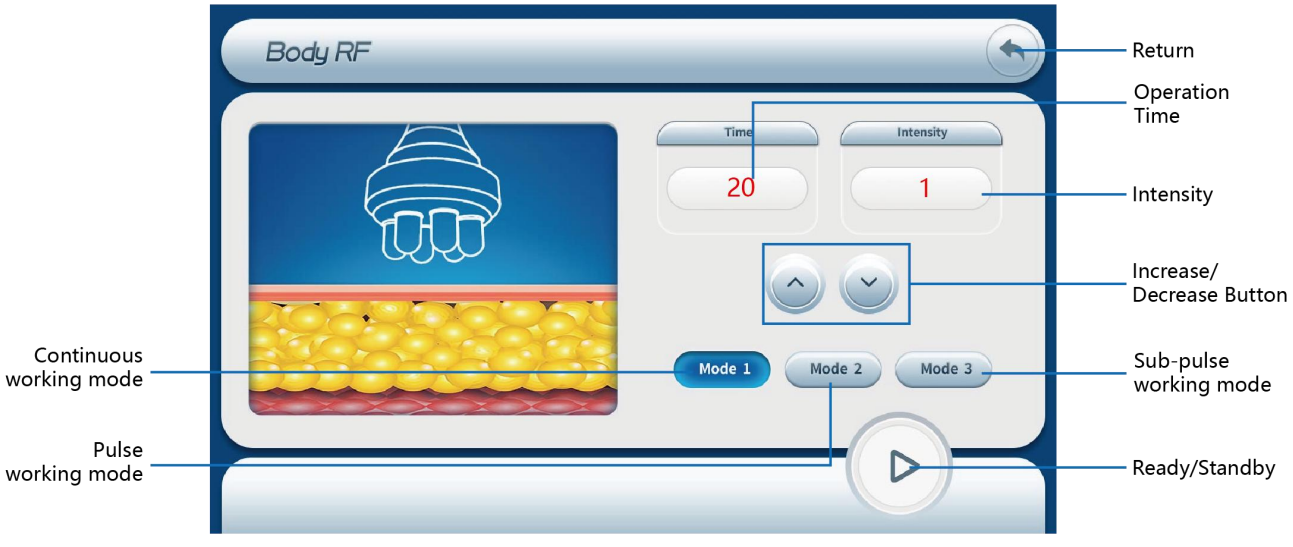

(3-2)

Click the RF Body button on the (1-2) interface to enter the (3-2) interface. It is recommended to set the time between 20-30 minutes, starting the energy from level 1. Adjust the energy level based on the customer's comfort. Mode 1 is the default mode, and you can also choose different modes based on the actual situation. Click start to begin

Interface introduction

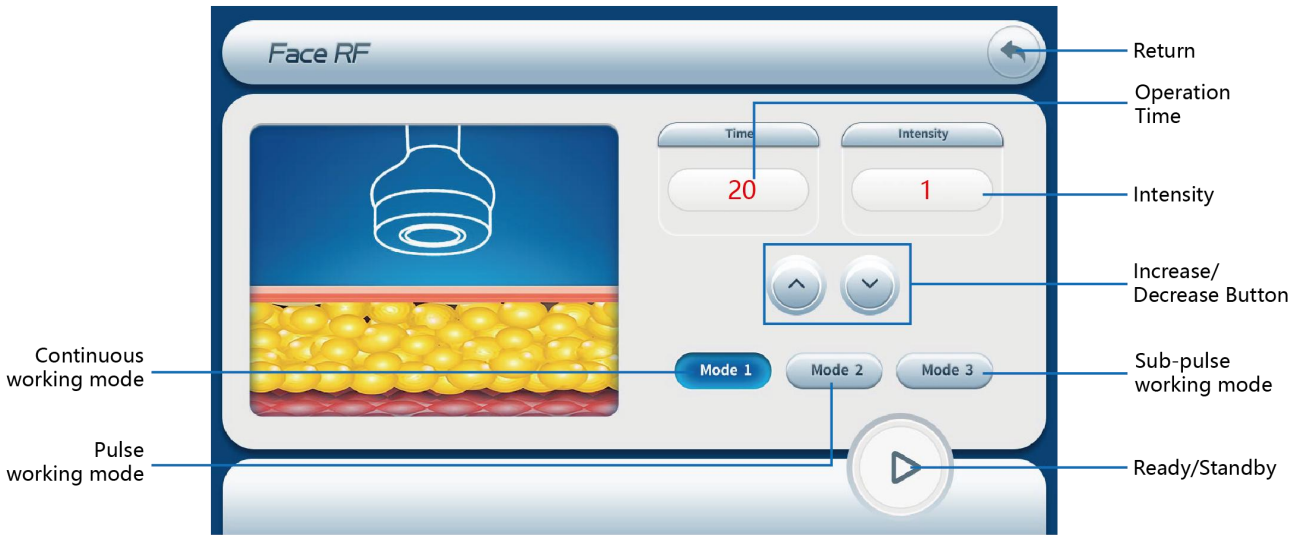

(3-3)

Click the RF Facial button on the (1-2) interface to enter the (3-3) interface. It is recommended to set the time between 20-30 minutes, starting the energy from level 1. Adjust the energy level based on the customer's comfort. Mode 1 is the default mode, and you can also choose different modes based on the actual situation. Click start to begin

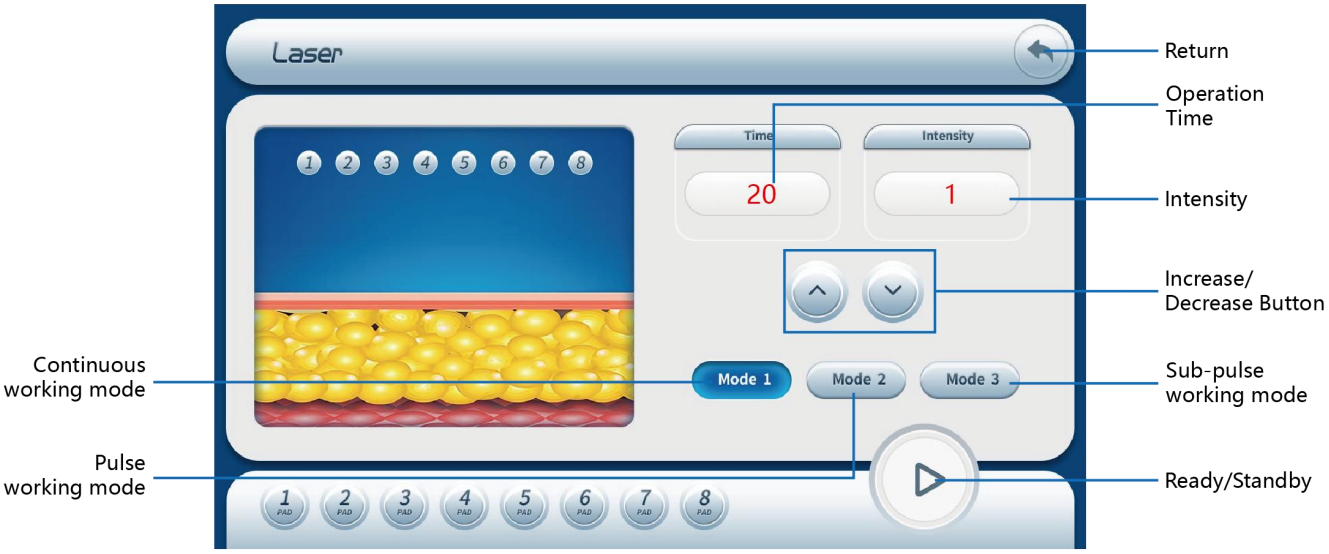

(3-4)

Click the LIPO button on the (1-2) interface to enter the (3-4) interface. It is recommended to set the time between 20-30 minutes, starting the energy from level 1. Adjust the energy level based on the customer's comfort. Mode 1 is the default mode, and you can also choose different modes based on the actual situation. Click start to begin

Instruction for use

Parameters setting table (adjust based on patient's feedback during the treatment)

Handle		Treatment Project Instructions	Parameter
Big size/Middle size Cryo handle	1# silicone applicator	Used for body areas with more pronounced curves or narrower body parts such as the waist, sides, and back	Set the cycle count to 1; Set the time to 15 minutes; Set the temperature to -10; Adjust the suction to 0.5 Adjust the release to 0.2, Parameters can be adjusted based on different treatment types and customer feedback
	2# silicone applicator	Suitable for areas with a thicker layer of fat, such as the abdomen.	
	3#/4# silicone applicator	Suitable for areas where the body fat is more vertical and the fat layer is relatively shallow, such as the thighs and arms	
Mini Cryo handle		Suitable for the chin or contour areas.	
RF-body handle		Suitable for overall body slimming	Start from 1
RF-face handle		Facial lifting and tightening	Start from 1
40K Handle		Suitable for overall body slimming	Start from 1
Lipo laser Pad	Large Lipo laser Pad	Applicable on the abdomen, waist, and thighs.	Start from 1
	Small Lipo laser Pad	Suitable for use on the arms and narrow areas of the body.	Start from 1

Instruction for use

Intended Users

The ideal candidates for 360-degree cryolipolysis are individuals with overall good health who are not satisfied with traditional methods of weight loss through diet and exercise or those seeking localized fat reduction without considering surgical options, such as liposuction. Clinical studies indicate that cryolipolysis is an effective method for reducing fat layers, offering noticeable and natural slimming results without the pain, risks, and recovery time associated with invasive procedures.

Contraindications

1. Hernia;
2. Abnormal bleeding;
3. Pregnancy or lactation;
4. Wearing pacemakers and defibrillators;
5. Recent surgery or presence of scar tissue;
6. Post-herpetic neuralgia or diabetic neuropathy;
7. Impaired skin sensation, compromised circulation around the treatment area;
8. Cold agglutinin disease, paroxysmal cold hemoglobinuria;
9. Chronic pain, patients with cold sensitivity or anxiety disorders;
10. Cold sensitivity conditions (e.g., cold urticaria or Raynaud's disease);
11. Open or infected wounds, eczema, dermatitis, or skin rash.

Instruction for use

Precautions

1. Avoid overeating and maintain a light diet, preferably choosing foods with lower calories and sugar content.
2. Take good care of the treated area for fat reduction. After the fat reduction procedure, the skin tissue in the treated area is relatively fragile. Avoid excessive pressure and consider using cold compresses for soothing to prevent symptoms such as bruising and unevenness.
3. Maintain a regular routine and stable mental and emotional well-being.

Accessories List

Large cryo handle	**2**
Medium cryo handle	2
Chin cryo handle	1
40KHz cavitation handle	1
RF-body Handle	1
RF-face Handle	1
Lipo Laser Pad (2pcs small, 6pcs large)	8
Straps (2pcs short, 3pcs medium, 3pcs long)	8
Anti-Freezing Membrane	5
Large Silicone Applicator	4
Medium Silicone Applicator	4